

User manual



grain special fruit moisture meter

humimeter FS4


1. Place the empty provided cup (0.5 litre) on the scale and turn the scale on. It shows 0.0 gram.






2. Make sure that the measuring chamber is completely empty. It is important that no material is left in the measuring chamber when you turn on the device.


3. Switch on the humimeter FS4 by pressing the power button () for 3 sec.

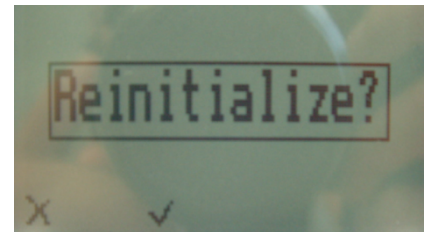

4. The next step is a self calibration. The word “reinitialize” will show up on your display. Accept by pressing the  button.



5. Select the right calibration curve for your material under test using the buttons  or .

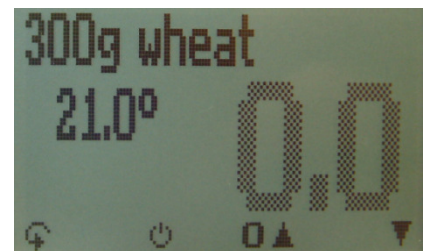

6. Fill up the cup with the sample material (+/- 1.0g). The filling quantity needed is shown on the upper left corner of the display of your device.



7. Fill up the measuring device with the sample material. The filling needs to be done slowly and constantly to ensure reproducible results.






8. The display shows the measuring result.




9. If the measuring value is blinking, the valid measuring range has been exceeded (limits see list on page 5). In this case the accuracy is decreasing.



10. To save the results in the store menu press  (▲ button). Storage was successful when the number in front of the symbol  increases. To reach the store menu please press (☛) until the  appears.



11. To name the saved results press the  button.




12. Empty the humimeter and ensure that no grain rests are accumulated in the measuring chamber.

Changing the batteries


Your new device is provided with batteries. Please find enclosed the manual for changing of batteries:

At first remove the rubber protective housing. For that, hold the rubber housing at the upper side and pull it over. If your humimeter is provided with an optional USB port, you have to remove the protection cap before. Press with your finger onto the arrow of the battery cap und pull it back.


Remove the empty batteries. Put four new batteries in the device. Make sure that the position of the battery poles is correct. Press down the batteries and close the cap.

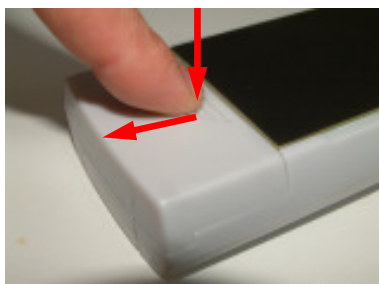



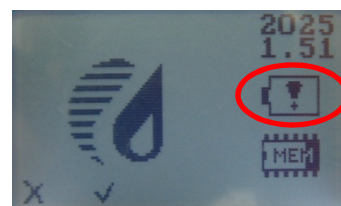


If the battery symbol appears in the measuring window resp. if a critical charge of battery is shown in the status, the batteries have to be changed IMMEDIATELY.

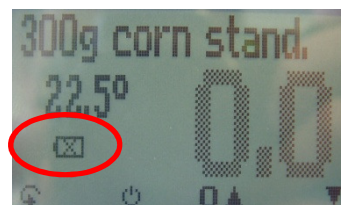

If you do not use your humimeter device for a longer period, remove the batteries. For eventual resulting damages we cannot provide any warranty.











List of calibration curves

Press the  or  key in the measuring window for at least 3 seconds and a list with all available sorts will appear. Select your sort by pressing  or  and confirm using the  key. The measurement will continue automatically.



Kennlinien


300g corn 5..40% 	300g hard corn 5..40% 	300g rye 5..28% 	300g triticale 5..28% 
300g wheat 5..28% 	300g durum 5..28% 	300g spelt peeled 5..28% 	300g barley 5..28% 
190g oats 5..25% 	300g rape 5..18% 	230g pumpkin seeds 2..20% 	310g peas 5..25% 
300g soybeans 9..18% 	295g horse beans 10..20% 	277g scarlet runner 8..25% 	180g sunflower 5..18% 
300g rice peeled 9..25% 	250g rice unpeeled 4..30% 	300g rice brown 4..26% 	300g buckwheat 5..18% 

300g millet 5..15% 	300g sorghum millet 5..25% 	200g jatropha 5..18% 	285g raw coffee peeled 9..18% 
180g raw coffee unpeeled 5..40% 	160g coffee roasted 1..20% 	150g coffee kibbled 2..10% 	300g poppy 5..15% 
10 pcs. free curves Special products can be calibrated or existing curves can be entered!	reference only for internal use!		

Empty calibration curves:

- The measuring device offers 10 empty calibration curves. They can be used for special fruits or variety calibration.
- On request Schaller GmbH can develop customized calibration curves for your product.

Design of the device

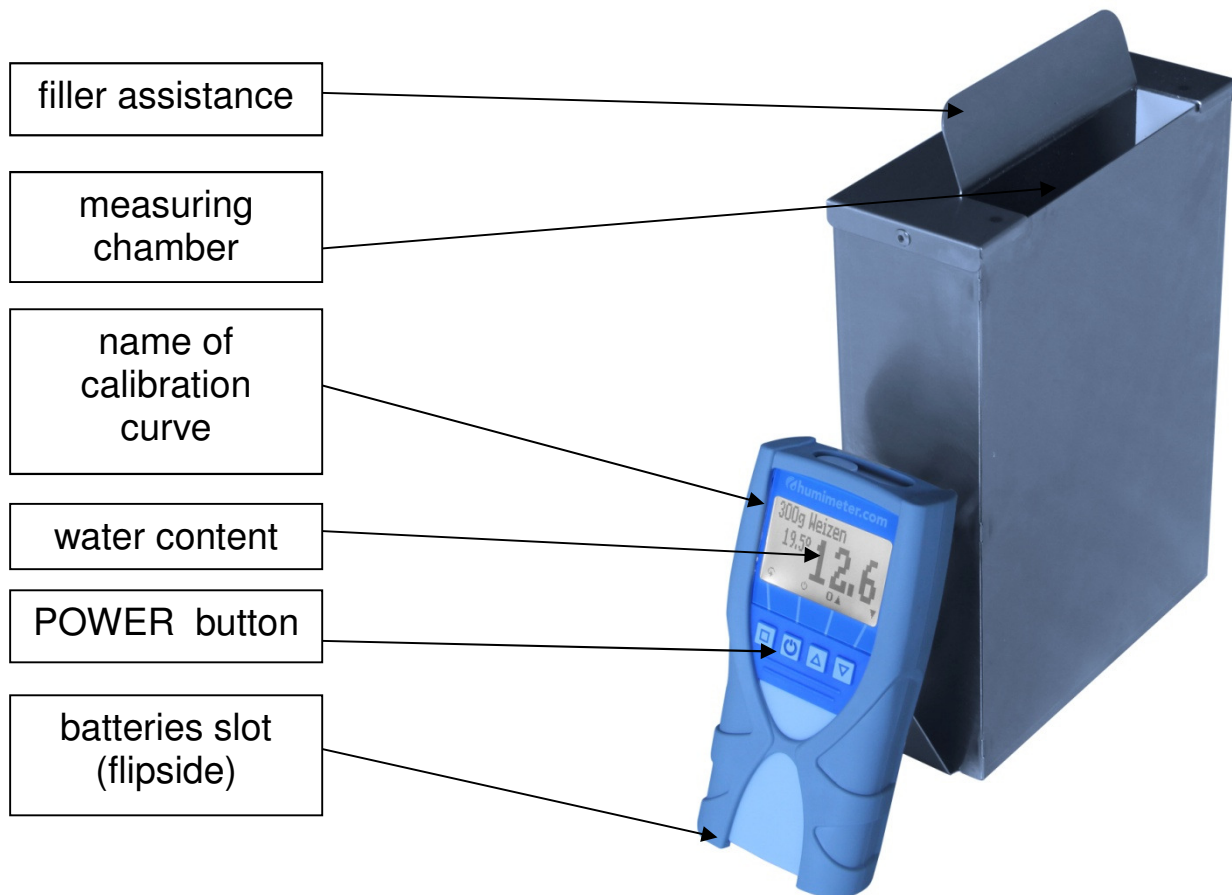

Determination of the material reference moisture

The principle is a comparison measurement with the dehydration method according to **EN ISO712**. Take the measured sample and weigh it. Dry it out in an oven and weigh it again.


$$\%F = \frac{M_n - M_t}{M_n} \times 100$$

M_n : Mass with average moisture content

M_t : Mass of the dried sample

%F: Calculated moisture content

Menu level overview

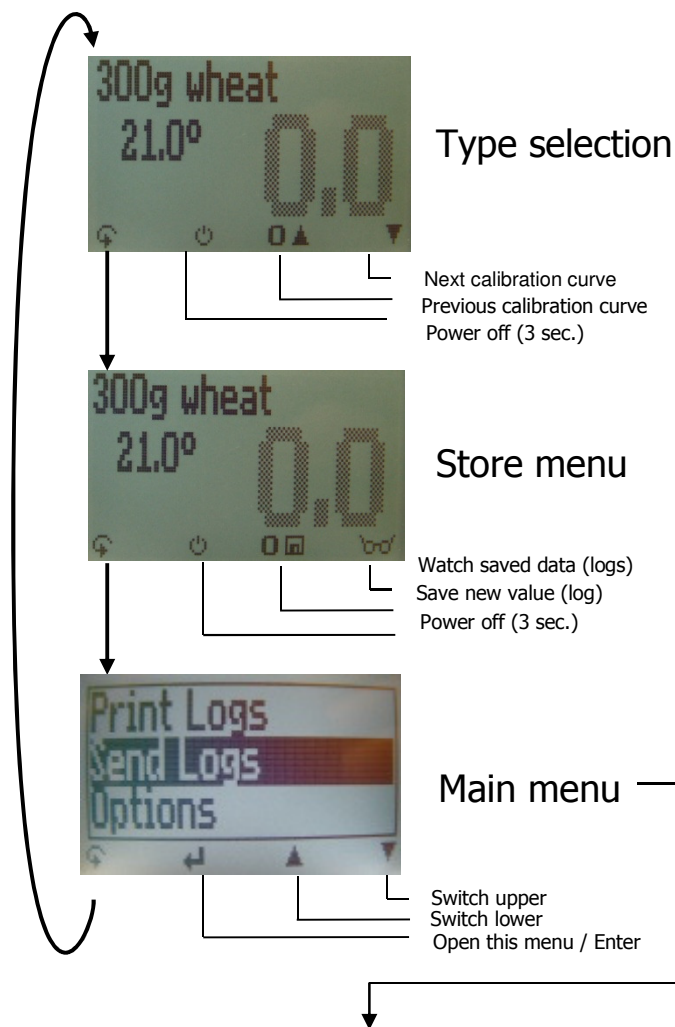

Overview main menu

<i>Edit Logs</i>	<i>Options</i>
Manual Logs	Date / Time
Clear Logs	Log Time
<i>Print Logs</i>	Language
Last Log	Unlock
All Logs	°C / °F
Clear Logs	BL On Time
<i>Send Logs</i>	Auto Off Time
Manual Logs	Materialcalib.
Clear Logs	o Online Send
<i>Options</i>	o Online Print
<i>Status</i>	Password
	Reset

Keypad symbols

Measuring window:

- Rolling Menu
- Power ON / OFF
- Switch upper
- Switch lower
- Save
- Hold
- Watch saved data
- Add suppliers data

Menu:

- Enter
- Switch upper
- Switch lower
- Exit
- Enter numbers
- Enter letters
- Next or right
- Left
- Yes
- No
- Shift
- OK

Transfer saved data to the PC




To send your saved logs to the PC, connect the humimeter device to your PC using the USB cable that was delivered with your device. Carefully loose the protection cap on your humimeter and plug in the USB mini B connector. The bigger connector has to be connected to a USB slot on your PC.



Start the LogMemorizer software on your PC and switch on your humimeter BM2.

The data transfer can be started on your humimeter or on the software.



Starting the data transfer on the humimeter:

Press the  key until you reach the menu (see image on the right). Then choose „Send Logs“ and confirm by pressing the  key. Now choose „Manual Logs“ and confirm with  again. All saved logs will be sent to your PC.

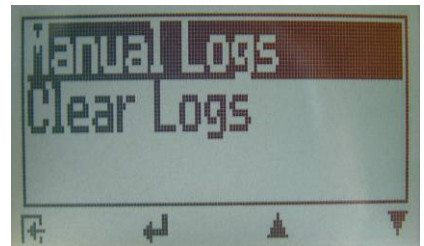
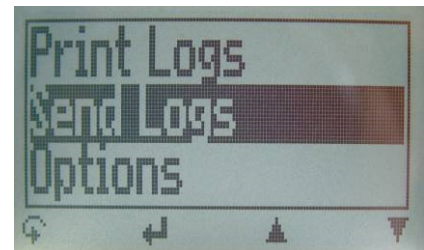


Starting the data transfer on your PC:

Press the button „communication“ in the LogMemorizer software. A menu with several options opens (see image below).

For transferring the data you can select „get last manual log“ (the last saved measuring series is transferred) or „get all manual logs“ (all saved logs are transferred).


If you click on one of these buttons, the transfer starts immediately.

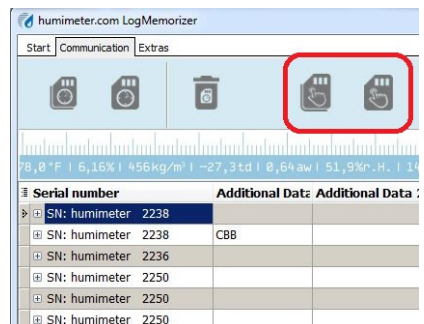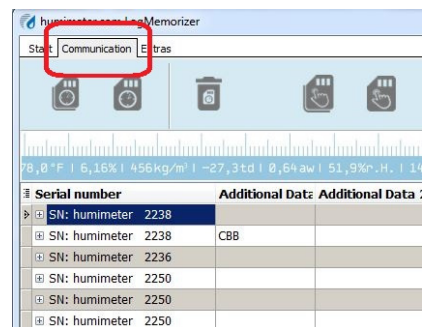



For the basic adjustments of the software please look through the instructions on the LogMemorizer USB flash drive.


Print saved data

To print your saved data, connect the device to the printer using the printer cable that was delivered with your device. Carefully loose the protection cap on the humimeter. At first plug in this side of the connector having the plastic casing closer to the end at the humimeter. Then switch on the device.



Not till then the other side of the cable has to be plugged in at the printer. Switch on the printer by pressing . Now the green LED is blinking. If it does not blink, please change the batteries and try again.

Press the  button at your humimeter until you reach the menu (see image on the right). Choose „Print Logs“ and confirm by pressing .


Now you can select a print of the last saved measuring series or of all saved measuring series (logs).


Confirm by pressing  again. The selected logs are printed out now.

To save paper, please think of clearing the data storage regularly.

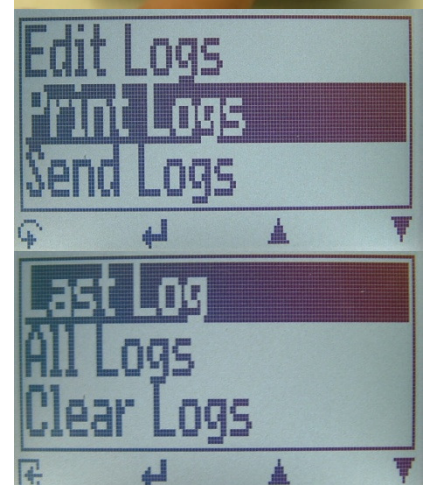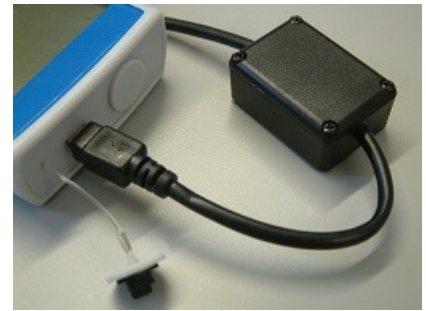

Online Print and Online Send

Your device supports the functions “Online Print” and “Online Send”. These functions can be activated in the menu „Options“. If an option is active, every newly recorded log will immediately be printed or transferred to the PC after pressing the  key.

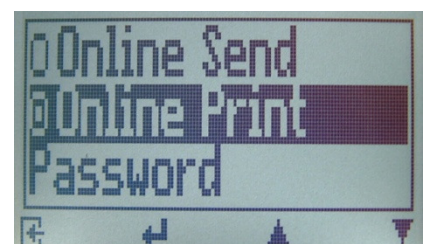

[illegible]

[illegible]



This image shows a full page of white paper with horizontal dashed lines, typical of primary-ruled notebook paper. The lines are evenly spaced and run across the width of the page. There are no margins, text, or other markings on the paper.

Exemption from liability

For miss-readings and wrong measurements and of this resulting damages we refuse any liability. This is a device for the quick determination of moisture. The moisture depends on multiple conditions and multiple materials. Therefore we recommend a plausibility check of the measuring results. Each device includes a serial number and the guarantee stamp. If those are broken, no claims for guarantee can be made. In case of a faulty device, please contact Schaller GmbH (www.humimeter.com) or our dealer.

Activation of the “super user” function

2 times  - *Options* – Unlock

Enter the 4-digit password by using the  button (standard is the 4-digit serial number) and confirm by pressing the  button.

Technical data

Resolution of the display	0.1% water content 0.5 °C temperature
Measuring range	0 up to 50% depending on the material
Operation temperature	0 up to +40 °C (32 up to 104 °F)
Storage temperature	-20 °C to +60 °C
Temperature compensation	automatically
Power supply	4 pcs. 1.5 Volt AA <u>Alkaline</u> batteries (900 measurements)
Auto Switch OFF	after app. 6 minutes
Current consumption	60mA (with light)
Display	128x64 matrix display, lighted
Dimensions	260 x 70 x 250 mm
Weight	approx. 1.3 kg (with batteries)
Degree of protection	IP 40
Scope of supply	FS4 incl. plastic case digital scale (max.500g, 0.1g) measuring cup 0.5 liter 4 pcs. 1,5Volt AA Alkaline bat. USB interface for PC transfer LogMemorizer software
Optional accessories	portable thermo printer

Device maintenance instructions

To provide a long life of your device please does not expose it to strong mechanical loads or heat e.g. dropping it or direct sunlight exposure. Clean your device using a dry cloth. The measuring chamber needs to be cleaned with a dry and soft brush.

Any kind of wet cleaning damages the device. The instrument is not rainproof. Keep it in dry areas. When the device is not used for a longer period (6 months) or when the batteries are empty, they should be removed to prevent a leakage of the battery acid.

! IMPORTANT ! please read

Most common reasons for miss readings

- ***Product temperature out of application range***

Material of a temperature **below 0°C** resp. **above +40°C** (32 to 104 °F) may cause faulty measurements. The storage of cold material in a warm storage area usually creates condensed water which may lead to major measuring errors.

- ***Not adjusted material under test***

Let your humimeter adjust to the surrounding temperature of the material for approx. half an hour.

A very high temperature difference has a negative effect on the stability of the measurement results.

- ***Wrong calibration curve***

Before measuring your sample please double-check the correct selection of the calibration curve.

- ***Wrong filling quantity***

Fill in exactly the right weight ($\pm 1.0\text{g}$) of material in the measuring chamber.

- ***Wet or mouldy material***

- ***Stored and fermented corn silage from whole grains may lead to higher value***

- ***Frozen measuring material***

- ***Polluted measuring material***

Polluted material e.g. barley spikes or other material mixed with the sample has a negative effect on the measurement